

1.601
1.363
1.340
1.316

2.354
2.168

3.830

4.278
4.255

7.679
7.625
7.324
7.298
7.271
7.260
7.130
7.105
7.103
7.050
7.042
7.037
6.950
6.947
6.941
6.923
6.920
6.450
6.396
5.296

Current Data Parameters
NAME vp070115.3eq4
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20150107
Time 15.20
INSTRUM spect
PROBHD 5 mm QNP 1H/13
PULPROG zg30
TD 32768
SOLVENT CDCl3
NS 16
DS 2
SWH 6172.839 Hz
FIDRES 0.188380 Hz
AQ 2.65542580 sec
RG 912.3
DW 81.000 usec
DE 6.50 usec
TE 298.2 K
D1 2.0000000 sec
TD0 1

==== CHANNEL f1 =====
NUC1 1H
P1 10.35 usec
PL1 -6.00 dB
SF01 300.1315000 MHz

F2 - Processing parameters
SI 32768
SF 300.1300063 MHz
WDW no
SSB 0
LB 0.00 Hz
GB 0
PC 1.00



Current Data Parameters
NAME vp070115.3
EXPNO 2
PROCNO 1

F2 - Acquisition Parameters
Date_ 20150107
Time 15.30
INSTRUM spect
PROBHD 5 mm QNP 1H/13
PULPROG jmod
TD 32768
SOLVENT CDC13
NS 129
DS 4
SWH 18832.393 Hz
FIDRES 0.574719 Hz
AQ 0.8700404 sec
RG 13004
DW 26.550 usec
DE 6.50 usec
TE 298.2 K
CNST2 145.0000000
CNST11 1.0000000
D1 2.00000000 sec
d20 0.00689655 sec
DELTA 0.00000700 sec
TD0 1

==== CHANNEL f1 =====
NUC1 13C
P1 5.50 usec
p2 11.00 usec
PL1 0.00 dB
SFO1 75.4747490 MHz


==== CHANNEL f2 =====
CPDPRG2 waltz16
NUC2 1H
PCPD2 100.00 usec
PL2 -3.00 dB
PL12 17.00 dB
SFO2 300.1312005 MHz

F2 - Processing parameters
SI 65536
SF 75.4677756 MHz
WDW EM
SSB 0
LB 3.00 Hz
GB 0
PC 1.40

166.25
159.52
144.44
142.16
135.40
129.76
129.53
128.91
128.60
128.49
127.80
124.90
122.78
122.14
120.74
120.57
119.57
114.59
111.84

77.48
77.05
76.63
59.76
54.78

20.91
13.64
13.40

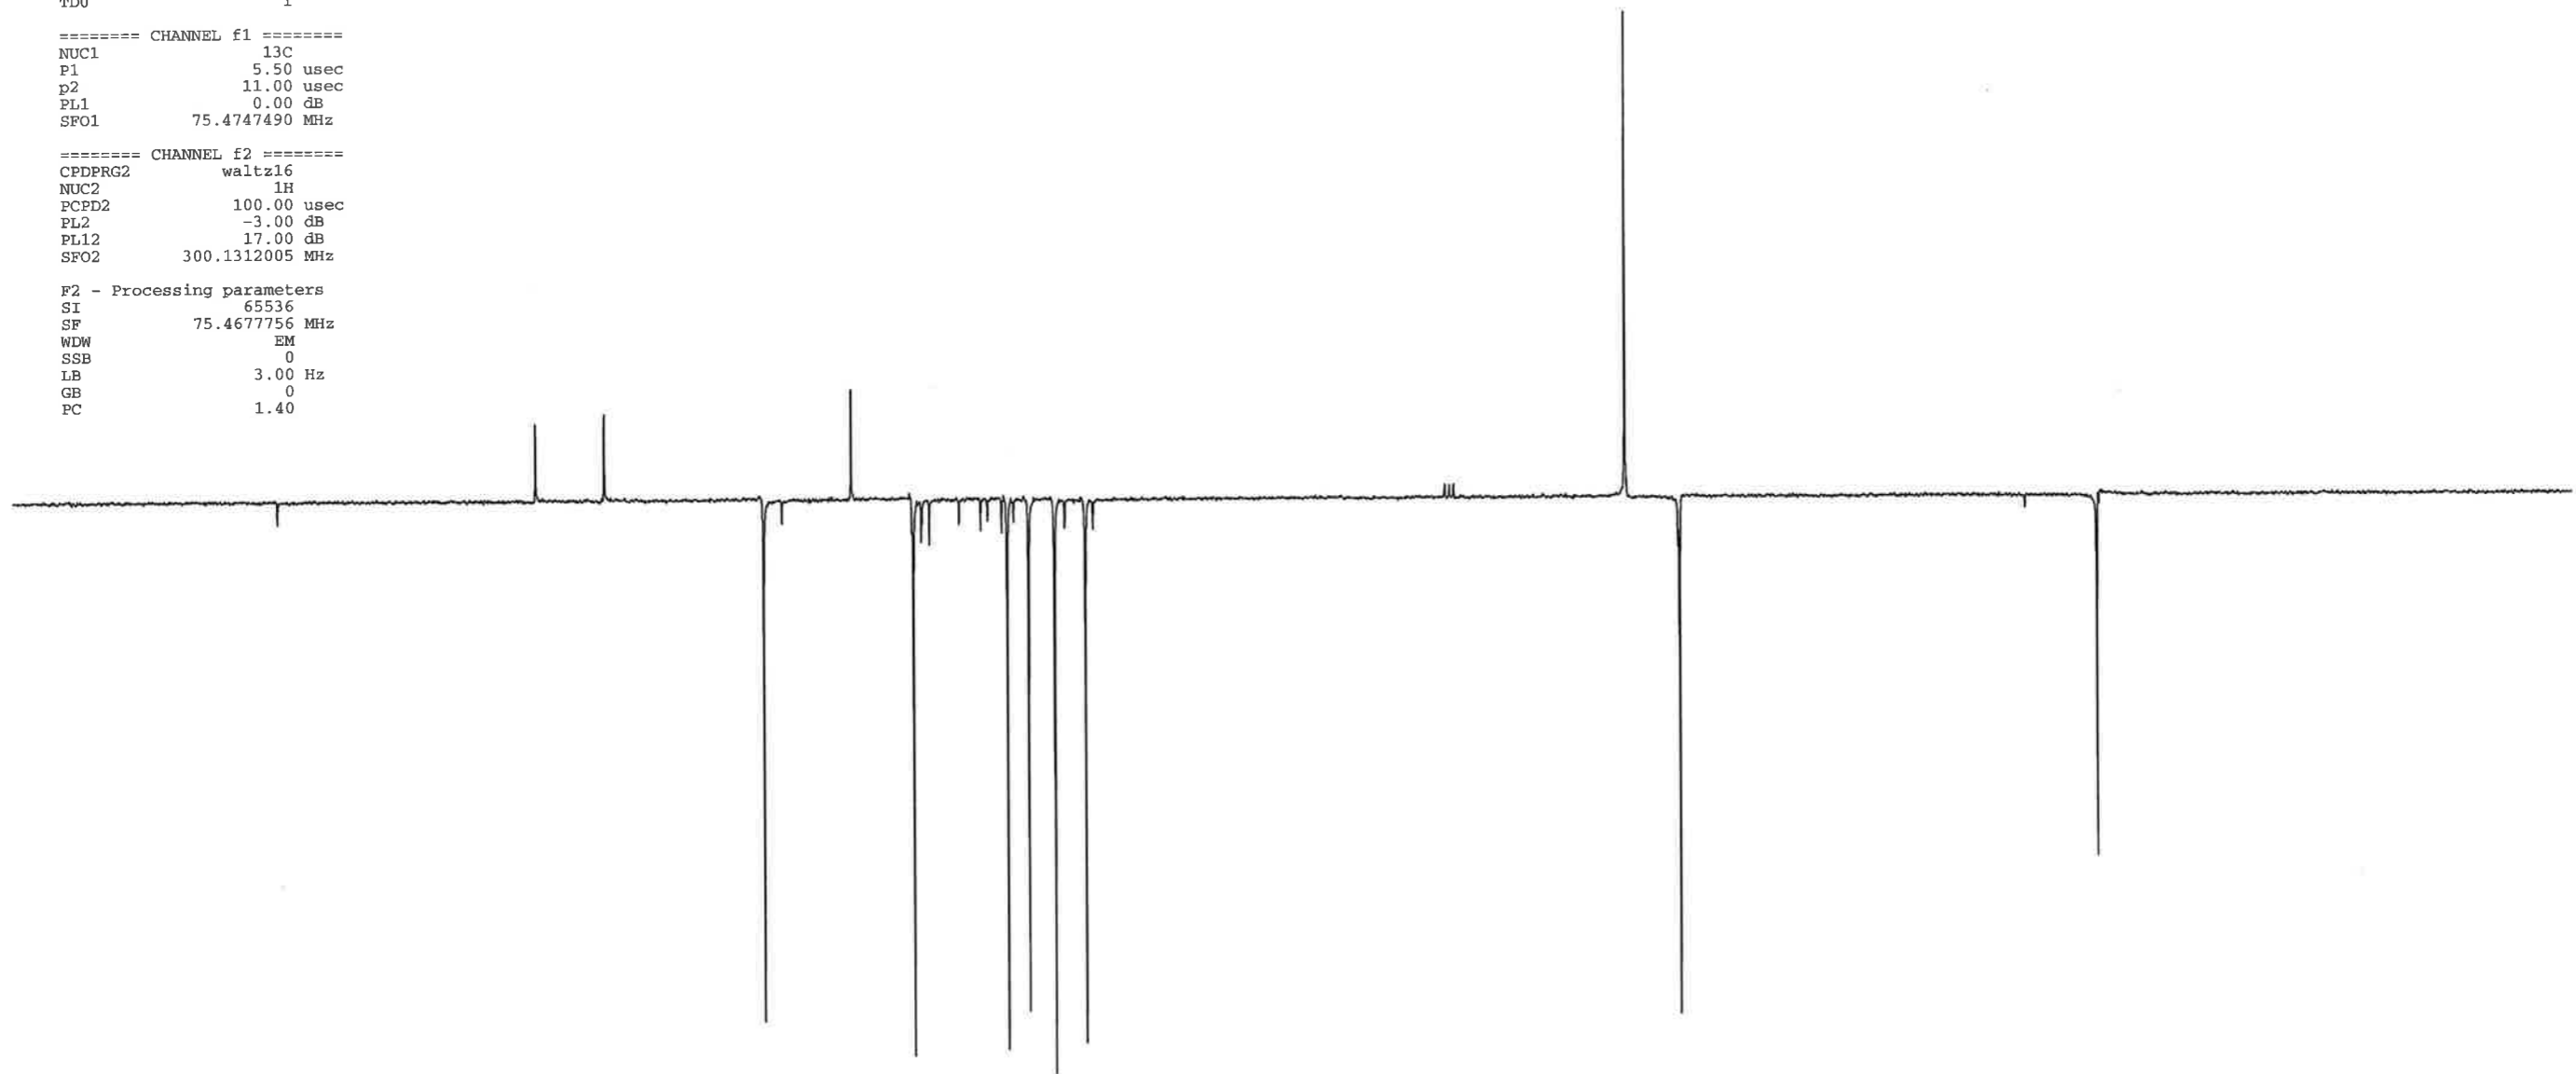

210 200 190 180 170 160 150 140 130 120 110 100 90 80 70 60 50 40 30 20 10 0 -10 -20 ppm